

Circulation

JOURNAL OF THE AMERICAN HEART ASSOCIATION



Apicoaortic Valve Containing Conduit in a Patient With Relapsing Prosthetic Endocarditis

Thomas Strecker, Dieter Ropers, Michael Weyand and Albrecht Reimann

Circulation 2007;116:e88-e89

DOI: 10.1161/CIRCULATIONAHA.107.692640

Circulation is published by the American Heart Association, 7272 Greenville Avenue, Dallas, TX 75214

Copyright © 2007 American Heart Association. All rights reserved. Print ISSN: 0009-7322. Online ISSN: 1524-4539

The online version of this article, along with updated information and services, is located on the World Wide Web at:

<http://circ.ahajournals.org/cgi/content/full/116/4/e88>

Data Supplement (unedited) at:

<http://circ.ahajournals.org/cgi/content/full/116/4/e88/DC1>

Subscriptions: Information about subscribing to *Circulation* is online at

<http://circ.ahajournals.org/subscriptions/>

Permissions: Permissions & Rights Desk, Lippincott Williams & Wilkins, a division of Wolters Kluwer Health, 351 West Camden Street, Baltimore, MD 21202-2436. Phone: 410-528-4050. Fax: 410-528-8550. E-mail:

journalpermissions@lww.com

Reprints: Information about reprints can be found online at

<http://www.lww.com/reprints>

Apicoaortic Valve–Containing Conduit in a Patient With Relapsing Prosthetic Endocarditis

Thomas Strecker, MD; Dieter Ropers, MD; Michael Weyand, MD; Albrecht Reimann, MD

A 58-year-old man with a history of 2 previous aortic valve replacements, one of which was a single vein graft to the right coronary artery, was referred to our hospital for repair of relapsing prosthetic endocarditis with annular abscess (Figure 1 and Data Supplement Movie I).

The patient was again taken to the operating theater, where a median sternotomy was performed and cardiopulmonary bypass was installed through aorto-right atrium cannulation. Intraoperatively, the need for the implantation of an apicoaortic conduit arose from both the profound paravalvular leakage and the inability to implant a new aortic valve prosthesis. The left ventricular outflow tract was closed with a patch of bovine glutaraldehyde-fixed pericardium (Figure 2). A circumferential Teflon ring with an adherent 30-mm Hemashield conduit and a 27-mm St. Jude Medical aortic valve-

carrying Hemashield conduit was sewn onto the left ventricular apex at 1 end and in an end-to-side fashion into the ascending aorta at the other (Figure 3). The reason for the insertion in the ascending aorta was to guarantee sufficient coronary perfusion.

Two months after the operation, 3- and 4-dimensional views of the heart taken by computed tomography and echocardiography show the functional apicoaortic valve-containing conduit (Figure 4 and Data Supplement Movies II through V).

Disclosures

None.

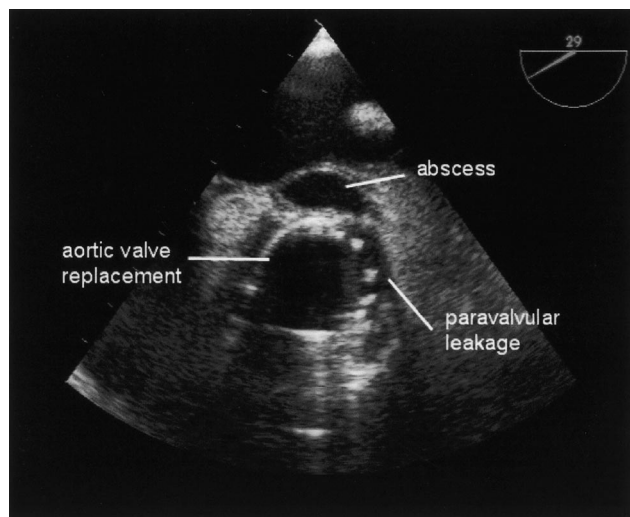


Figure 1. Transesophageal echocardiography reveals a giant circular paravalvular leakage and an abscess formation around the prosthetic aortic valve. The annulus was almost completely destroyed.

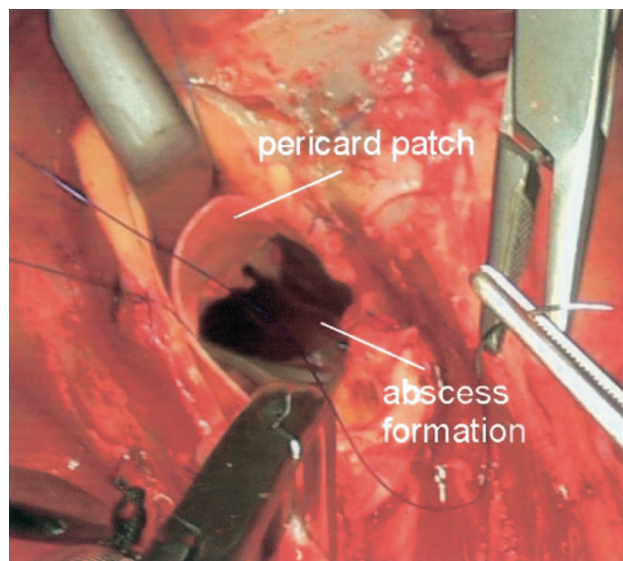


Figure 2. Intraoperative photograph shows the inside of the abscess formation on the left ventricular outflow tract, which was closed with a patch of bovine glutaraldehyde-fixed pericardium.

From the Center of Cardiac Surgery (T.S., M.W., A.R.) and the Department of Cardiology (D.R.), Friedrich-Alexander-University of Erlangen-Nuremberg, Erlangen, Germany.

The online-only Data Supplement, which contains movies, can be found at <http://circ.ahajournals.org/cgi/content/full/116/4/e88/DC1>.

Correspondence to Thomas Strecker, MD, Center of Cardiac Surgery, Friedrich-Alexander-University of Erlangen-Nuremberg, Krankenhausstr 12, D-91054 Erlangen, Germany. E-mail thomas.strecker@herz.imed.uni-erlangen.de

(*Circulation*. 2007;116:e88-e89.)

© 2007 American Heart Association, Inc.

Circulation is available at <http://www.circulationaha.org>

DOI: 10.1161/CIRCULATIONAHA.107.692640

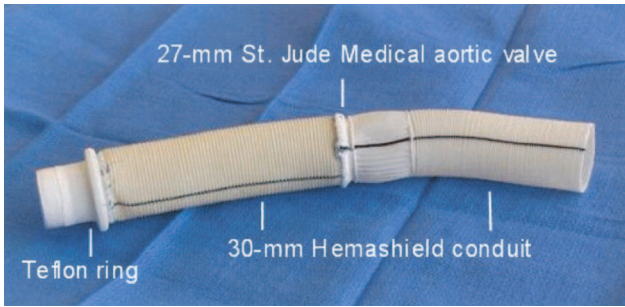


Figure 3. Intraoperative photograph of the apicoaortic valve-containing conduit taken before implantation. The conduit consists of a circumferential Teflon ring with an adherent 30-mm Hemashield conduit and a 27-mm St. Jude Medical aortic valve-carrying Hemashield conduit.

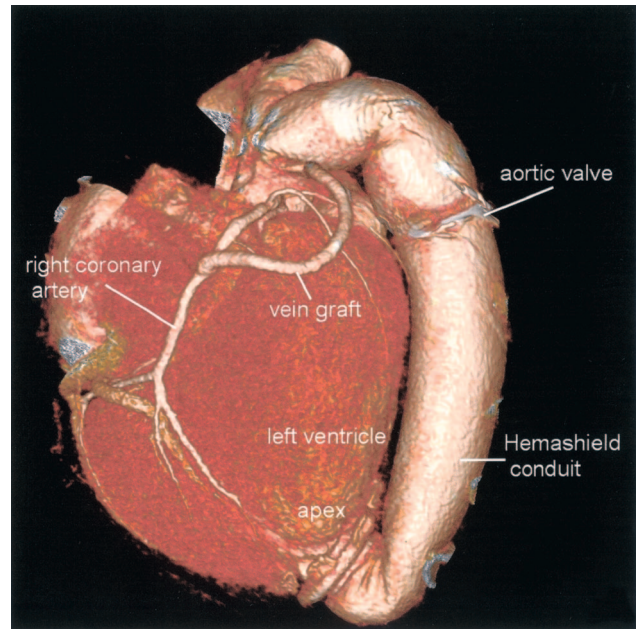


Figure 4. Visualization of the apicoaortic valve-containing conduit as well as the previous bypass graft to the right coronary artery by 64-slice row spiral multidetector computed tomography reconstruction.